

Bioprinting of Corning® Matrigel® Matrix with the Corning Matribot® Bioprinter: Evaluating the Precision of the Temperature-controlled Syringe Pump Printhead

CORNING

Application Note

Introduction

Corning Matrigel matrix is commonly used in 3D cell culture, as it provides structure and signaling cues necessary for 3D and organoid models. In these models, Matrigel matrix is typically either used to coat the bottom of a microplate surface or it is dispensed as droplets to form domes. This latter method, which is commonly used when working with precious samples such as organoids, can be time-consuming and variable between users due to the Matrigel matrix's viscosity and temperature sensitivity.

The Corning Matribot bioprinter is a 3D bioprinter that contains a temperature-controlled printhead, enabling an ideal system for Matrigel matrix dispensing. This syringe-based system can be used to accurately and precisely dispense small volumes of hydrogels with or without cells in a semi-automated throughput. Here we demonstrate the precision and accuracy of the Matribot bioprinter for dispensing Matrigel matrix as 10 μL and 50 μL droplets.

Materials and Methods

Corning Matrigel matrix solution with a protein concentration of 9 mg/mL was dispensed as single droplets into pre-weighed weigh boats using the Corning Matribot bioprinter dispense parameters listed in Table 1. The volume of each dispensed droplet, as represented by mass, was measured by determining the mass difference of the weigh boat before and after Matrigel matrix addition.

Results and Discussion

When programming a target volume of 10 μL droplets of 9 mg/mL Corning Matrigel matrix in the Corning Matribot bioprinter, we were able to dispense 9.63 ± 0.80 mg of Matrigel matrix droplets with a coefficient of variation (CV) of 8.3% and systematic error under 4% (Table 2 and Figure 1).

When programming a target volume of 50 μL droplets of 9 mg/mL Corning Matrigel matrix in the Corning Matribot Bioprinter, we were able to dispense 49.16 ± 1.39 mg of Matrigel matrix droplets with a CV of 2.8% and systematic error under 2% (Table 2 and Figure 2).

Table 1. Conditions for dispensing 10 μL and 50 μL droplets of 9 mg/mL Corning Matrigel matrix solution.

Target volume	10 μL	50 μL
Nozzle type	27G needle, 0.5"	27G needle, 0.5"
Volume loaded in 3 mL syringe	2.5 mL	2.6 mL
Set temperature in printhead	0°C	0°C
Set temperature of printbed	37°C	37°C
Room temperature	23°C	23°C
Volume purged before experiment	200 μL	200 μL
Distance between nozzle and substrate	1 mm	1 mm
Sample size	48	47

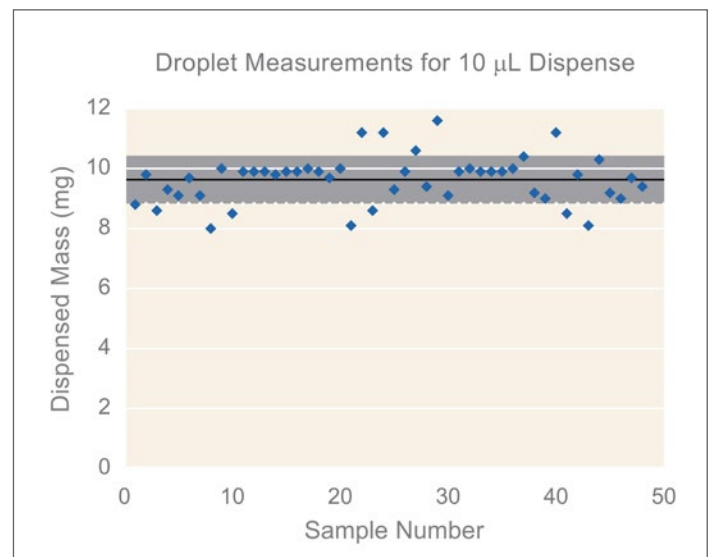


Figure 1. The dispensed droplet volume for 10 μL dispensing of 9 mg/mL Corning Matrigel matrix as measured by mass. The average mass for 48 dispenses is represented by a black line and the standard deviation is shown by gray shading.

Table 2. Mean dispensed mass from dispensing 10 μL and 50 μL droplets of 9 mg/mL Corning Matrigel matrix solution.

Target volume	10.00 μL	50.00 μL
Mean dispensed mass	9.63 mg	49.16 mg
Standard Deviation	0.80 mg	1.39 mg
Trueness/systematic error	3.7 %	1.7 %
% CV	8.3	2.8

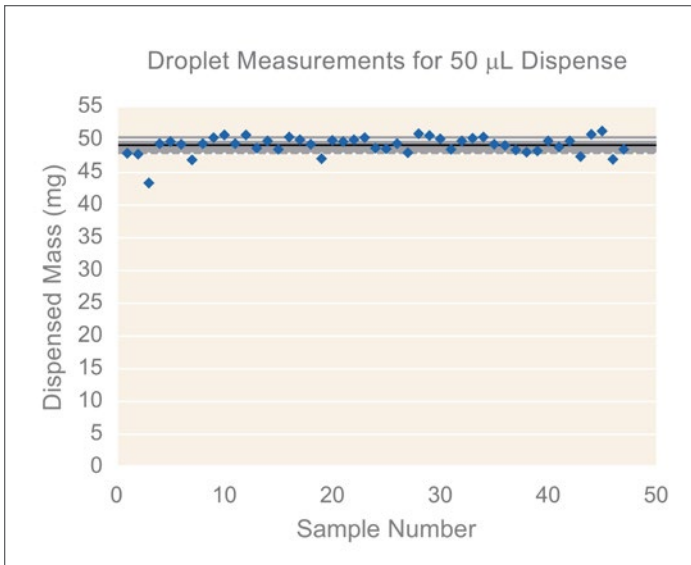


Figure 2. The dispensed droplet volume for 50 µL dispensing of 9 mg/mL Corning Matrigel matrix as measured by mass. The average mass for 47 dispenses is represented by a black line and the standard deviation is shown by gray shading.

To determine systematic error (% SE)

$$\bar{V} = \frac{1}{N} \sum_{i=1}^N V_i \quad \%SE = \frac{\bar{V} - V_T}{V_T} \times 100\%$$

\bar{V} is the average of all measured volumes;

N is the number of replicate deliveries;

V_i is a single measured volume;

V_T is the target volume, the volume intended to be delivered.

To determine random error (% CV)

$$\%CV = \frac{100\%}{\bar{V}} \sqrt{\frac{\sum_{i=1}^N (V_i - \bar{V})^2}{N - 1}}$$

Warranty/Disclaimer: Unless otherwise specified, all products are for research use or general laboratory use only.* Not intended for use in diagnostic or therapeutic procedures. Not for use in humans. These products are not intended to mitigate the presence of microorganisms on surfaces or in the environment, where such organisms can be deleterious to humans or the environment. Corning Life Sciences makes no claims regarding the performance of these products for clinical or diagnostic applications. *For a listing of US medical devices, regulatory classifications or specific information on claims, visit www.corning.com/resources.

Conclusions

The Corning® Matrigel® matrix solution dispensed by the temperature-controlled syringe pump printhead as measured by mass matched the target volumes with a high accuracy and reproducibility.

We also found the dispensing precision to be dependent on the target volume, where it has a higher precision for a volume of 50 µL (CV of 2.8%) compared to 10 µL (CV of 8.3%). In both cases, the systematic error was well below 5%, indicating the robustness of this bioprinting technology.

CORNING

Corning Incorporated
Life Sciences

www.corning.com/lifesciences

NORTH AMERICA
t 800.492.1110
t 978.442.2200

ASIA/PACIFIC
Australia/New Zealand
t 61 427286832
Chinese Mainland
t 86 21 3338 4338

India
t 91 124 4604000
Japan
t 81 3-3586 1996
Korea
t 82 2-796-9500
Singapore
t 65 6572-9740
Taiwan
t 886 2-2716-0338

EUROPE
CSEurope@corning.com
France
t 0800 916 882
Germany
t 0800 101 1153
The Netherlands
t 020 655 79 28
United Kingdom
t 0800 376 8660

All Other European Countries
t +31 (0) 206 59 60 51

LATIN AMERICA
grupoLA@corning.com
Brazil
t 55 (11) 3089-7400
Mexico
t (52-81) 8158-8400