

Corning® BioCoat® Matrigel® Invasion Chambers

Frequently Asked Questions

CORNING

The Corning BioCoat Matrigel Invasion Chamber is a useful tool to study the invasion of malignant cells. For cells to metastasize, they must be able to secrete proteases that break down the basement membrane as well as migrate. Invasion through a Corning Matrigel matrix-coated cell culture insert has become the gold standard for low throughput quantitative and qualitative measurement of cellular metastatic potential, including investigation of the mechanisms of cell invasion and inhibition of cell invasion¹⁻¹⁰.

1. How do I prepare Corning BioCoat Matrigel invasion chambers for use?

Remove the package from storage at -20°C and allow it to come to room temperature.

Confirm that the inserts are in the notches of the companion plates. Add warm bicarbonate-based media to the interior of the inserts. For exact volumes, see Corning BioCoat Matrigel Invasion Chamber Guidelines for Use (SPC-354480-G, enclosed with the product). Allow to rehydrate for two hours in a 5% CO₂ incubator.

NOTE: If you do not want to use all the inserts in the same experiment, do not allow them to thaw, as repeated freeze-thaws will damage the Matrigel matrix barrier. Open the package under aseptic conditions, and, using sterile forceps, transfer the inserts to a separate companion plate to thaw. Wrap the unused inserts in the original packaging and quickly return them to the -20°C freezer.

2. Should I add chemoattractant into the upper or lower chambers?

The chemoattractant should be placed in the lower, or basolateral, chamber. It slowly diffuses into the upper, or apical, chamber setting up a chemotactic gradient for the cells to follow. See Corning BioCoat Matrigel Invasion Chamber Guidelines for use for detailed instructions.


3. Does it matter if I have air bubbles, and how do I prevent them?



It is critical that the BioCoat Matrigel invasion chambers are in the notches and there are no air bubbles. Add pre-warmed media containing chemoattractant to the wells of the Falcon® tissue culture companion plate, or add just media to the negative control wells. Use sterile forceps to transfer the chambers into the previously filled wells of the companion plate. To avoid air bubbles, tip the chamber at a slight angle as it is lowered into the liquid and align the notches. If there are air bubbles, carefully tap the side of the plate to dislodge the bubbles.

4. I don't want cells to be weak during the migration/invasion assay, so can I add serum to the upper chambers?

We do not recommend adding serum to the apical chamber; try using 0.1% BSA instead. We recommend starting with bovine serum albumin. If you must add serum to the apical compartment, use 0.4%. High concentrations of serum in the apical compartment interfere with the chemotactic gradient.

Air Bubble

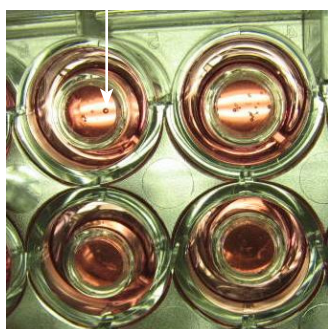

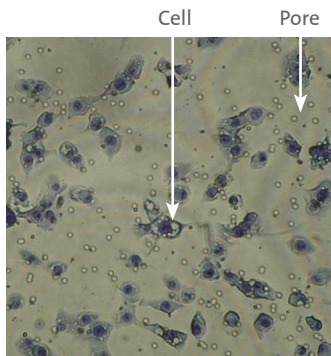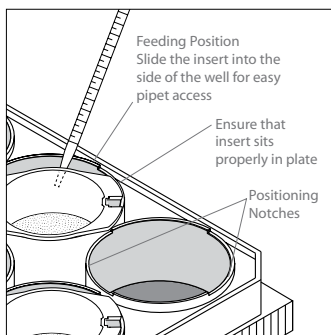

5. I used Corning® BioCoat® Matrigel® invasion chambers and the Corning BioCoat control inserts, but the cells were uneven on the bottom of the insert. Why did this happen?

There will be some normal variability, and you should count multiple fields. All conditions should be run in triplicate. Always check for air bubbles when setting up your assay, because cells will not migrate through the dry patches. Always use Falcon® 24-well cell culture insert companion plates that come with the system (Corning 353504) and Falcon 6-well cell culture insert companion plates (Corning 353502)—do not use standard multiwell plates. Make sure the inserts are in the positioning notches of the companion plates.

6. What will the cells look like under the microscope?

Cells will look slightly different depending on the cell type. The cells will have an irregular shape. The pores will be round or ovoid and be refractile.

7. If incubation times are long, do cells proliferate after migration/invasion?

We recommend doing a migration control on uncoated inserts and calculating the percent invasion by dividing the number of cells that invaded through the Corning Matrigel invasion chamber by the number of cells that migrated through the control insert and multiplying by 100. This controls for proliferation. See the Corning BioCoat Matrigel Invasion Chamber Guidelines for use for details.

8. What reagent do you recommend for staining the cells on the membrane?

We recommend any colorimetric stain that differentially stains the cytoplasm and the nucleus such as hematoxylin and eosin (H&E) or Wrights stain. Two examples of these types of stains are Diff-Quik™ (VWR 47733-150) and Hemacolor® Stain Set (Merck KGaA 65044-93).

9. Are there any tips to wipe off the Matrigel matrix from the insert?

You should remove the liquid from the top of the insert and pre-wet the cotton swab. Hold the insert at an angle so the bottom of the membrane is not touching a flat surface and gently swab out the gel, taking care to remove the cells but not detaching the insert membrane from the housing.

10. How can I remove the membrane? Do you supply a special blade?

Do not remove the membrane from the housing until the staining is complete. A special blade is not supplied. Use a #11 scalpel to cut the membrane from the housing and immediately mount cell-side down on a microscope slide. Put a drop of immersion oil on the membrane, and cover it with a coverslip.

11. How long can I keep the hydrated insert? Is it possible to store for several days after the hydration?

You should use the rehydrated insert after the normal 2-hour rehydration period. If you must use it the next day because your cells are not ready expect the CV between replicates to increase. Do not use after 24 hours.

12. I did not get very much invasion of my cells, what should I do?

Verify, with an inverted microscope, that the invaded cells have not detached from the bottom of the insert and have fallen to the bottom well.

Since there is no serum in the seeding media, make sure you either use a non-enzymatic method of removing the cells prior to seeding, or do a serum wash to deactivate the trypsin. Make sure you are using the notched Falcon 24-well cell culture insert companion plates (Corning 353504) and Falcon 6-well cell culture insert companion plate (Corning 353502) and that the cell culture inserts are in the notches. Verify there are no air bubbles trapped under the inserts.

Different cell types invade at different rates, and the protocol may need to be adjusted for different cell types. As a first step, increase the serum concentration to 10% in the lower chamber and increase the cell number to 50,000 cells per 24-well insert or 250,000 cells per 6-well insert. If this does not increase the raw invasion numbers sufficiently, you can increase the invasion time from 24 to 48 hours.

The Corning BioCoat Matrigel invasion chamber is highly cited in the scientific literature with specific details for many cell types. You can contact Corning Life Sciences Scientific Support for assistance in locating a reference for your specific cell type.

References

1. Kong D, et al. Inhibition of angiogenesis and invasion by 3,3'-diindolylmethane is mediated by the NF- κ B downstream target genes MMP-9 and uPA that regulated bioavailability of VEGF in prostate cancer. *Cancer Res.* 67(7):3310 (2007).
2. Albini A and Benelli R. The chemoinvasion assay: a method to assess tumor and endothelial cell invasion and its modulation. *Nat. Protocols.* 2(3):505 (2007).
3. Oxelmark E, et al. The cochaperone p23 differentially regulates estrogen receptor target genes and promotes tumor cell adhesion and invasion. *Mol. Cell Biol.* 26(14):5205 (2006).
4. Duxbury MA, et al. EphA2: a determinant of malignant cellular behavior and a potential therapeutic target in pancreatic adenocarcinoma. *Oncogene.* 23:1448 (2004).
5. Seton-Regers SE, et al. Cooperation of the ErbB2 receptor and transforming growth factor in induction of migration and invasion in mammary epithelial cells. *Proc. Natl. Acad. Sci.* 101(5):1257 (2004).
6. Singh A, et al. CXCL12-CXCR4 interactions modulate prostate cancer cell migration, metalloproteinase expression and invasion. *Lab. Invest.* 84:1666 (2004).
7. Takada Y, et al. Evodiamine abolishes constitutive and inducible NF- κ B activation by inhibiting I κ B α kinase activation, thereby suppressing NF- κ B-regulated antiapoptotic and metastatic gene expression, up-regulating apoptosis, and inhibiting invasion. *J. Biol. Chem.* 280(17):17203 (2005).
8. Ichikawa H, et al. Identification of a novel blocker of I κ B α kinase that enhances cellular apoptosis and inhibits cellular invasion through suppression of NF κ B-regulated gene products. *J. Immunol.* 174(11):7383 (2005).
9. Silvera D, et al. Essential role for eIF4G1 overexpression in the pathogenesis of inflammatory breast cancer. *Nat. Cell Biol.* 11:903-908 (2009).
10. Kajiro M, et al. The ubiquitin ligase CHIP acts as an upstream regulator of oncogenic pathways. *Nat. Cell Biol.* 11:312-319 (2009).

Warranty/Disclaimer: Unless otherwise specified, all products are for research use or general laboratory use only.* Not intended for use in diagnostic or therapeutic procedures. Not for use in humans. These products are not intended to mitigate the presence of microorganisms on surfaces or in the environment, where such organisms can be deleterious to humans or the environment. Corning Life Sciences makes no claims regarding the performance of these products for clinical or diagnostic applications. *For a listing of US medical devices, regulatory classifications or specific information on claims, visit www.corning.com/resources.

Corning's products are not specifically designed and tested for diagnostic testing. Many Corning products, though not specific for diagnostic testing, can be used in the workflow and preparation of the test at the customers discretion. Customers may use these products to support their claims. We cannot make any claims or statements that our products are approved for diagnostic testing either directly or indirectly. The customer is responsible for any testing, validation, and/or regulatory submissions that may be required to support the safety and efficacy of their intended application.

CORNING

Corning Incorporated
Life Sciences

www.corning.com/lifesciences

NORTH AMERICA

t 800.492.1110
t 978.442.2200

ASIA/PACIFIC

Australia/New Zealand

t 61 427286832

Chinese Mainland

t 86 21 3338 4338

India

t 91 124 4604000

Japan

t 81 3-3586 1996

Korea

t 82 2-796-9500

Singapore

t 65 6572-9740

Taiwan

t 886 2-2716-0338

EUROPE

CSEurope@corning.com

France

t 0800 916 882

Germany

t 0800 101 1153

The Netherlands

t 020 655 79 28

United Kingdom

t 0800 376 8660

All Other European Countries

t +31 (0) 206 59 60 51

LATIN AMERICA

grupoLA@corning.com

Brazil

t 55 (11) 3089-7400

Mexico

t (52-81) 8158-8400