

Generating Lentiviral Particles in the Corning® HYPERFlask® Cell Culture Vessel

CORNING

SnAPPShots

A brief technical report
from the Corning
Applications Group

Katherine E. Strathearn, Ph.D.,
and Mark E. Rothenberg, Ph.D.
Corning Life Sciences
Kennebunk, Maine 04043

Introduction

Lentiviruses are enveloped retroviruses that are becoming major biological tools in cell therapy applications. These types of retroviruses are unique for their ability to (a) deliver a stable gene(s) into most non-dividing cells, (b) integrate their genetic cargo into a target chromosome, and (c) increase their versatility by modifying various molecular properties (e.g., modification of glycoproteins around the envelope) (1). To allow researchers and manufacturers the opportunity to produce even higher yields in the same spatial footprint as a T-175 flask, Corning offers the HYPERFlask vessel. The HYPERFlask Cell Culture Vessel features Corning's HYPER (High Yield PERFORMANCE) technology which consists of a gas permeable film that serves as the attachment surface and eliminates the headspace within a vessel. This allows for an increase in the number of layers and corresponding cell growth surface area, as compared to traditional rigid single layer culture vessels. The HYPERFlask Vessel cell growth surface area is 1,720 cm² across 10 layers, and has the same spatial footprint of a T175 vessel.

Lentiviral particles are produced when cells (e.g., HEK-293LTV) are transfected with DNA encoding various genes (e.g., genes encoding viral packaging and envelope proteins) needed for lentivirus propagation. The focus of this study was to determine the efficacy of generating virus using the unique Corning HYPER technology compared to traditional T-flask vessels. Utilizing the HYPERFlask vessel, researchers can generate higher yields in a smaller spatial footprint that saves time and space. The results described here demonstrate that the experimental approach to generate lentivirus in the HYPERFlask vessel led to equivalent titers and higher yields compared to that generated using a standard T-175 flask.

Methods and Materials

Cell Culture

HEK-293LTV cells (Cell BioLabs, Cat. No. LTV-100) were maintained in DMEM with sodium pyruvate (Corning cellgro,® Cat. No. 10-013-CM), 10% FBS (Corning cellgro, Cat. No. 35-010-CV), and 1X MEM Nonessential Amino Acids (Corning cellgro, Cat. No. 25-025-Cl).

DNA preparation

GC10 competent cells (Sigma-Aldrich,® Cat. No. G2544) were heat shocked with the DNA obtained from the ViraSafe™ Lentiviral Bicistronic Expression System (GFP), Pantropic (Cell BioLabs, Cat.

No. VPK-218-PAN) and pLenti-GFP Lentiviral Control Vector (Cell BioLabs, Cat. No. LTV-400), and cultured in LB-Broth (Corning cellgro, Cat. No. 46-050-CM) in a 1L Erlenmeyer flask (Corning Cat. No. 431403) at 37°C for 16 h at 250 rpm. Plasmid DNA was purified using the AxyPrep™ Plasmid Maxiprep kit (Axygen, Cat. No. AP-MX-P-25) and quantified with the EnVision® multimode plate reader (Perkin Elmer).

Preparation of the DNA:CaPO₄ Complex

On the day of transfection, a master mix of DNA containing CaPO₄ was prepared based on a total growth area of 1945 cm² (1720 cm² [HYPERFlask] + 175 cm² [comparison T-175] + 50 cm² [extra]). To prepare the mix, 19 mL of freshly made 2X HBS buffer (50 mM HEPES, 250 mM NaCl, 1.5 mM Na₂HPO₄, pH 7.07) was added to a 50 mL conical tube (Corning, Cat. No. 430921) labeled Tube A. To a separate 50 mL conical tube (Tube B), the following DNA components were added at a combined ratio of 0.55 µg/cm²:

- ▶ pLenti Green Fluorescent Protein (GFP) Control Vector (465 µg)
- ▶ pREV-RSV (packaging vector) (202 µg)
- ▶ pCgpV (packaging vector) (202 µg)
- ▶ pCMV-VSVG (envelope vector) (202 µg)

Cell culture grade water (Corning cellgro, Cat. No. 25-055-CV) and 1M CaCl₂ (Sigma-Aldrich,® Cat. No. 21115) were added to Tube B to yield a final volume of 19 mL, and incubated at room temperature for 5 minutes. Following the 5 minute incubation, the contents of Tube B were added dropwise to Tube A at a rate of approximately 5 mL/min, and incubated for 20 minutes at room temperature. After approximately one third of the CaCl₂-DNA solution had been added, the mixture would exhibit a cloudy appearance. Please note: if white precipitates form while mixing, then the solution in Tube B was added to Tube A either too quickly or with too much agitation. The formation of these precipitates greatly reduces the transfection efficiency. Each experiment was performed six times in replicate.

Transfection of HEK-293LTV Cells

Cells were seeded onto a T-175 Corning CellBIND® Surface flask (Corning, Cat. No. 431328) or Corning HYPERFlask® vessel (Corning, Cat. No. 10034) at 100,000 cells/cm² (0.326 mL/cm²) and incubated overnight at 37°C (5% CO₂, 98% relative humidity). The following day, 5 to 6 hours prior to the transfection, the media was removed and replaced with fresh media (0.326 mL/cm²) containing 25 µM chloroquine (Sigma, Cat. No. C6628). For optimal

transfection efficiency, the pH of the medium at the time of the transfection was between 7.5 to 7.6. To transfect the 293LTV cells, the medium containing chloroquine was removed from each vessel and combined into a 1L storage bottle (Corning, Cat. No. 430518). Thirty-seven mL of the medium was removed, and 37 mL of the DNA:CaPO₄ solution prepared above was added dropwise at a rate of approximately 7 mL/min. The medium containing the DNA:CaPO₄ solution was added slowly back to each vessel and incubated for 16 hours at 37°C (3% CO₂, 98% relative humidity). Following the incubation, the transfection medium was removed, fresh medium was added to the vessels and then collected 48 hours later. GFP expression was monitored throughout the course of the experiment using the AMG EVOS® FI microscope.

Lentivirus Harvest

Viruses can undergo a lytic or lysogenic life cycle. Lentiviruses undergo the lysogenic cycle, which results in the release of virus into the medium without cell lysis (Fig. 1). As a result, the medium was collected approximately 65 hours post transfection, and the cells were discarded. To remove any cell debris and multivesicular bodies (MVB), the medium was filtered through a 0.45 µm cellulose acetate filter (Corning, Cat. No. 430514 or 430627) and collected into an autoclaved glass bottle (Corning, Cat. No. 1395-1L or 1395-100). To concentrate the virus, 35 mL of the virus solution obtained from each vessel was transferred to a Spin-X® filter (MWCO 100,000) (Corning, Cat. No. 431491) and centrifuged at 3000 x g (4°C) until a final volume of ~300 µL was collected (two spin steps were performed to concentrate 35 mL). The lentiviruses encoding GFP (concentrated, and non-concentrated) were then aliquoted and stored at -80°C.

Lentivirus Titer

The Lenti-X™ qRT-PCR Titration Kit was purchased from Clontech (Cat. No. 631235), and the assay was performed according to manufacturer's instructions using the CFX96 Touch™ Real-Time PCR Detection System (Bio-Rad). The copies/mL were calculated based on the Cq values determined by the software.

Transduction of Vero and MDBK Cells

To verify that the virus was functional, Vero (ATCC,™ Cat. No. CCL-81) and Mardin-Darby Bovine Kidney (MDBK) (ATCC, Cat. No. CCL-22) cells were transduced. Previous titration results from FACS suggested that approximately 1,000 copies/mL is equivalent to 1 TU/mL (transduction unit/mL). Cells were seeded onto a 24-well plate (Corning, Cat. No. 3527) at 5,000 cells/cm² and incubated overnight at 37°C (5% CO₂, 98% relative humidity). The following day, the concentrated lentiviruses encoding GFP were added to the cells at a multiplicity of infection (MOI) of 20. Polybrene® (Sigma-Aldrich, Cat. No. H9268), at a final concentration of 10 µg/mL, was also added to the medium to improve lentivirus transduction efficiency. The amount of each virus (mL) added to each well was calculated using the following formula:

$$[(\text{Cells/cm}^2) \times (\text{cm}^2 \text{ of well}) \times (\text{MOI } 20 \text{ (TU/cells)})] / (\text{TU/mL})$$

The cells were harvested 72 hours later, and the GFP expression was analyzed by flow cytometry.




Figure 1. Schematic of Lentivirus production.

Flow Cytometry

To assess GFP expression, Vero and MDBK cells transduced with lentivirus encoding GFP were harvested, centrifuged to remove trypsin/media, and then resuspended in 500 µL of PBS (Corning cellgro,® Cat. No. 21-040-CM). Cell suspensions were analyzed using the MACSQuant® Analyzer instrument (Miltenyi Biotec).

Results

Cell Morphology and GFP Expression

To assess lentiviral production using a T-175 flask compared to a HYPERFlask vessel, HEK-293LTV cells were transfected with DNA obtained from the ViraSafe™ Lentiviral Bicistronic Expression System (GFP). GFP expression and cell morphology were monitored throughout the course of the experiment. The medium was collected approximately 65 hours post transfection. Similar cell morphology and GFP expression were observed in samples from both vessels (Fig. 2) throughout the course of the experiment.

Lentiviral Production

Once collected and filtered, the lentivirus' encoding GFP from each vessel were then titered using the Lenti-X™ qRT-PCR Titration Kit to determine copies/mL. Lentivirus obtained from the HYPERFlask vessel yielded similar copies/mL (Fig. 3A), similar copies/cm² (Fig. 3B), and approximately 10 times more copies (Fig. 3C) compared to lentivirus obtained from the T-175 flask. These results indicate that lentivirus particles may be generated in the HYPERFlask® vessel with similar titers, but larger yields are obtained when compared to a standard T-175 vessel with a similar spatial footprint.

GFP Expression in Vero and MDBK Cells

To verify that the virus obtained from the HYPERFlask® vessel was as functional as virus obtained from the T-175 flask, Vero and MDBK cells were transduced with lentivirus encoding GFP. Each cell type was transduced with virus obtained from either the HYPERFlask vessel or a T-175 flask at a MOI of 20. After 72 hours, the cells were collected and analyzed via flow cytometry. The average GFP fluorescence in each cell line infected with lentivirus was greater than 90.0% (Fig. 4, two independent experiments). Taken together, these results indicate that the HYPERFlask vessel produces similar infectious lentiviral particles per cm² compared to a traditional T-175 flask.

Summary

In summary, this study demonstrates the utility of the HYPER Technology as an alternative to traditional cell culture flasks for scale up production of Lentivirus.

- ▶ Lentiviral particles can be amplified in the Corning HYPERFlask vessel at similar titers compared to traditional tissue culture vessels, while allowing for greater virus production in a smaller footprint.

- ▶ Lentiviral particles generated on the HYPER technology platforms also exhibit similar levels of infection compared to traditional culture vessels.
- ▶ Furthermore, the HYPER technology platform of products includes larger vessels with larger surface areas that provide researchers with the ability to further increase Lentivirus production.




Figure 2. Analysis of GFP expression in the Corning HYPERFlask. Representative images from the same experiment demonstrating similar GFP expression in the Corning HYPERFlask and T-175 Flask. Scale bar represents 1000 μm . These trends were observed with all experiments. Images were captured using the AMG EVOS® FI microscope.

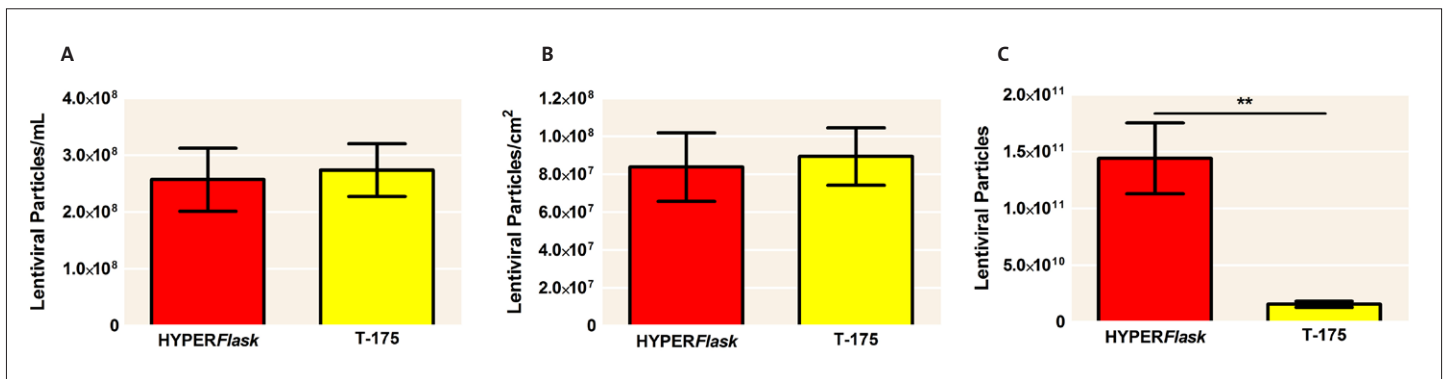


Figure 3. The Corning HYPERFlask vessel supports comparable viral production, with a higher yield of total virus compared to a T-175 flask. (A) Titers obtained from the Lenti-X™ qRT-PCR Titration Kit. (B) When normalized on a per cm^2 basis the HYPERFlask vessel yields similar amount of lentiviral particles. (C) The HYPERFlask vessel generates a significantly higher amount of total infectious adenoviral particles. Paired t-test, ** $p < 0.01$, $N=6$.





Figure 4. Vero and MDBK cells transduced with Lentivirus exhibit comparable levels of GFP expression. Representative flow cytometry data. Expression of GFP (green) compared to a negative control of non-transduced cells (black). After two independent experiments, the GFP expression in both the Vero or MDBK cells was greater than 90%, regardless of which vessel in which the virus was generated.

Reference

- Giry-Laterrière, M., Verhoeyen, E., and Salmon, P. Viral Vectors for Gene Therapy: Methods and Protocols, *Methods Mol. Biol.* 2011. 737:183-209.

For additional product or technical information, please visit www.corning.com/lifesciences or call 1.800.492.1110. Outside the United States, please call **978.442.2200** or contact your local Corning sales office listed below.



www.corning.com/lifesciences/solutions

At Corning, cells are in our culture. In our continuous efforts to improve efficiencies and develop new tools and technologies for life science researchers, we have scientists working in Corning R&D labs across the globe, doing what you do every day. From seeding starter cultures to expanding cells for assays, our technical experts understand your challenges and your increased need for more reliable cells and cellular material.

It is this expertise, plus a 160-year history of Corning innovation and manufacturing excellence, that puts us in a unique position to offer a beginning-to-end portfolio of high-quality, reliable cell culture consumables.

Corning Incorporated Life Sciences

836 North St.
Building 300, Suite 3401
Tewksbury, MA 01876
t 800.492.1110
t 978.442.2200
f 978.442.2476

www.corning.com/lifesciences

Worldwide Support Offices

ASIA/PACIFIC

Australia/New Zealand
t 0402-794-347

China
t 86 21 2215 2888
f 86 21 6215 2988

India
t 91 124 4604000
f 91 124 4604099

Japan

t 81 3-3586 1996
f 81 3-3586 1291

Korea

t 82 2-796-9500
f 82 2-796-9300

Singapore

t 65 6733-6511
f 65 6861-2913

Taiwan

t 886 2-2716-0338
f 886 2-2516-7500

EUROPE

France

t 0800 916 882
f 0800 918 636

Germany

t 0800 101 1153
f 0800 101 2427

The Netherlands

t 31 20 655 79 28
f 31 20 659 76 73

United Kingdom

t 0800 376 8660
f 0800 279 1117

All Other European Countries

t 31 (0) 20 659 60 51
f 31 (0) 20 659 76 73

LATIN AMERICA

Brasil

t (55-11) 3089-7419
f (55-11) 3167-0700

Mexico

t (52-81) 8158-8400
f (52-81) 8313-8589

The Corning Family of Brands

CORNING **costar** **cellgro** **PYREX** **AXYGEN** **GOSSSELIN**

For a listing of trademarks, visit us at www.corning.com/lifesciences/trademarks. All other trademarks in this document are the property of their respective owners. Corning Incorporated, One Riverfront Plaza, Corning, NY 14831-0001